

Technical Note

## Highly Selective DNA-Based Sensor for Lead(II) and Mercury(II) Ions

Chi-Wei Liu, Chih-Ching Huang, and Huan-Tsung Chang

*Anal. Chem.*, **2009**, 81 (6), 2383-2387 • DOI: 10.1021/ac8022185 • Publication Date (Web): 16 February 2009

Downloaded from <http://pubs.acs.org> on March 29, 2009

### More About This Article

---

Additional resources and features associated with this article are available within the HTML version:

- Supporting Information
- Access to high resolution figures
- Links to articles and content related to this article
- Copyright permission to reproduce figures and/or text from this article

[View the Full Text HTML](#)



ACS Publications  
High quality. High impact.

# Highly Selective DNA-Based Sensor for Lead(II) and Mercury(II) Ions

Chi-Wei Liu,<sup>†</sup> Chih-Ching Huang,<sup>‡</sup> and Huan-Tsung Chang<sup>\*†</sup>

Department of Chemistry, National Taiwan University, 1, Section 4, Roosevelt Road, Taipei, Taiwan, and Institute of Bioscience and Biotechnology, National Taiwan Ocean University, 2, Beining Road, Zhongzheng District, Keelung, Taiwan

We have developed a technique for the highly selective and sensitive detection of Pb<sup>2+</sup> and Hg<sup>2+</sup> using a thrombin-binding aptamer (TBA) probe labeled with the donor carboxyfluorescein (FAM) and the quencher 4-([4-(dimethylamino)phenyl]azo)benzoic acid (DABCYL) at its 5' and 3' termini, respectively. The TBA has a random coil structure that changes into a G-quartet structure and a hairpin-like structure upon binding Pb<sup>2+</sup> and Hg<sup>2+</sup> ions, respectively. As a result, the fluorescence decreases through fluorescence resonance energy transfer (FRET) between the fluorophore and quencher. These changes in fluorescence intensity allow the selective detection of Pb<sup>2+</sup> and Hg<sup>2+</sup> ions at concentrations as low as 300 pM and 5.0 nM using this TBA probe in the presence of phytic acid and a random DNA/NaCN mixture, respectively. The linear correlation existed between the fluorescence intensity and the concentration of Pb<sup>2+</sup> and Hg<sup>2+</sup> over the range of 0.5–30 nM ( $R^2 = 0.98$ ) and 10–200 nM ( $R^2 = 0.98$ ), respectively. To the best of our knowledge, this is the first example of a single DNA-based sensor that allows the detection of both Hg<sup>2+</sup> and Pb<sup>2+</sup> ions. This simple and cost-effective probe was also applied to separately determine Pb<sup>2+</sup> in soil samples and spiked Hg<sup>2+</sup> in pond samples.

The monitoring of toxic metal ions in aquatic ecosystems is an important issue because these contaminants can have severe effects on human health and the environment.<sup>1</sup> Lead and mercury are two of the most toxic metallic pollutants; for example, lead can cause renal malfunction and inhibit brain development<sup>2</sup> and mercury can damage the brain, heart, and kidneys.<sup>3</sup> Although the powerful technique of inductively coupled plasma mass spectrometry (ICPMS) is used in most current protocols for the detection of these two metal ions, it is rather expensive, complex, and not

suitable for on-site analyses.<sup>4</sup> The past few years have witnessed great progress in the development of optical and electrochemical techniques for the detection of metal ions. Procedures using small molecules,<sup>5</sup> DNazymes,<sup>6</sup> oligonucleotides,<sup>7</sup> polymers,<sup>8</sup> and functional nanoparticles<sup>7c,9</sup> have all been developed for the selective detection of Pb<sup>2+</sup> and/or Hg<sup>2+</sup>. For example, a fluorescence resonance energy transfer (FRET)-based DNazyme system was demonstrated for Pb<sup>2+</sup> sensing. The sensor was made of FRET between fluorophore and quencher labeled on the DNazyme (17E) and its substrate, respectively. In the presence of Pb<sup>2+</sup>, the 17E catalyzes hydrolytic cleavage of substrate and it turned on the fluorescence for sensing.<sup>6</sup> For the detection of Hg<sup>2+</sup>, a colorimetric method was developed using DNA-modified gold nanoparticles (DNA–Au NPs) in aqueous media under a temperature control. In that assay, two types of DNA-functionalized Au NPs were prepared, each functionalized with different thiolated-DNA sequences (5' HS–C<sub>10</sub>–A<sub>10</sub>–T–A<sub>10</sub> 3' and 5' HS–C<sub>10</sub>–T<sub>10</sub>–T–T<sub>10</sub> 3'), which are complementary except for a single thymidine–thymidine mismatch. Each increase in concentration of 1.0 μM results in an increase in the melting point by about 5.0 °C, thus providing an easy way of determining Hg<sup>2+</sup> concentration.<sup>9d</sup> Nevertheless, many of these systems have limited practical use because of, for example, poor aqueous solubility, cross-sensitivity toward other metal ions, matrix interference, high cost (e.g., enzymes), complicated processing, the use of unstable molecules (e.g., RNA), or poor sensitivity. Previously, we unveiled a homoge-

\* To whom correspondence should be addressed. Phone and Fax: 011-886-2-33661171. E-mail: changht@ntu.edu.tw.

<sup>†</sup> National Taiwan University.

<sup>‡</sup> National Taiwan Ocean University.

- (1) (a) Campbell, L. M.; Dixon, D. G.; Hecky, R. E. *J. Toxicol. Environ. Health, Part B* **2003**, *6*, 325–356. (b) Needleman, H. *Annu. Rev. Med.* **2004**, *55*, 209–222.
- (2) Needleman, H. L. *Human Lead Exposure*; CRC Press: Boca Raton, FL, 1991.
- (3) (a) Hoyle, I.; Handy, R. D. *Aquat. Toxicol.* **2005**, *72*, 147–159. (b) Zalups, R. K. *Pharmacol. Rev.* **2000**, *52*, 113–143.

(4) Li, Y.; Chen, C.; Li, B.; Sun, J.; Wang, J.; Gao, Y.; Zhao, Y.; Chai, Z. *J. Anal. At. Spectrom.* **2006**, *21*, 94–96.

(5) (a) Deo, S.; Godwin, H. A. *J. Am. Chem. Soc.* **2000**, *122*, 174–175. (b) Nolan, E. M.; Lippard, S. J. *J. Am. Chem. Soc.* **2003**, *125*, 14270–14271. (c) Yang, Y.-K.; Yook, K.-J.; Tae, J. *J. Am. Chem. Soc.* **2005**, *127*, 16760–16761.


(6) (a) Li, J.; Lu, Y. *J. Am. Chem. Soc.* **2000**, *122*, 10466–10467. (b) Liu, J.; Lu, Y. *J. Am. Chem. Soc.* **2003**, *125*, 6642–6643. (c) Thomas, J. M.; Ting, R.; Perrin, D. M. *Org. Biomol. Chem.* **2004**, *2*, 307–312. (d) Xiao, Y.; Rowe, A. A.; Plaxco, K. W. *J. Am. Chem. Soc.* **2007**, *129*, 262–263.

(7) (a) Ono, A.; Togashi, H. *Angew. Chem., Int. Ed.* **2004**, *43*, 4300–4302. (b) Chiang, C.-K.; Huang, C. C.; Liu, C.-W.; Chang, H.-T. *Anal. Chem.* **2008**, *80*, 3716–3721. (c) Liu, C.-W.; Hsieh, Y.-T.; Huang, C.-C.; Chang, H.-T. *Chem. Commun.* **2008**, 2242–2244. (d) Babkina, S. S.; Ulakhovich, N. A. *Anal. Chem.* **2005**, *77*, 5678–5685.

(8) (a) Kim, I.-B.; Bunz, U. H. F. *J. Am. Chem. Soc.* **2006**, *128*, 2818–2819. (b) Geary, C. D.; Zudans, I.; Goponenko, A. V.; Asher, S. A.; Weber, S. G. *Anal. Chem.* **2005**, *77*, 185–192.

(9) (a) Huang, C.-C.; Chang, H.-T. *Chem. Commun.* **2007**, *12*, 1215–1217. (b) Huang, C.-C.; Chang, H.-T. *Anal. Chem.* **2006**, *78*, 8332–8338. (c) Huang, C.-C.; Yang, Z.; Lee, K.-H.; Chang, H.-T. *Angew. Chem., Int. Ed.* **2007**, *46*, 6824–6828. (d) Lee, J.-S.; Han, M. S.; Mirkin, C. A. *Angew. Chem., Int. Ed.* **2007**, *46*, 4093–4096.

### Scheme 1. Cartoon Representation of the Sensing Mechanism of the TBA Probe for the Detection of Hg<sup>2+</sup> and Pb<sup>2+</sup> Ions




neous assay using the DNA-binding dye TOTO-3 and polythymidine (poly-T) to detect Hg<sup>2+</sup> through T–Hg<sup>2+</sup>–T interactions, which induce a conformational change of poly-T into a folded structure that preferably binds TOTO-3.<sup>7b</sup> Although such optical (or electrochemical) sensing techniques can be sensitive and selective, they generally allow the detection of only one of the two metal ions.

In this paper we present a technique for the highly selective and sensitive detection of Pb<sup>2+</sup> and Hg<sup>2+</sup> using a thrombin-binding aptamer (TBA) probe<sup>10,11</sup> labeled with the donor carboxyfluorescein (FAM) and the quencher 4-([4-(dimethylamino)phenyl]azo)benzoic acid (DABCYL) at its 5' and 3' termini, respectively. The sensing mechanism of this probe is based on the change in the DNA strand's conformation from the linear to a folded structure upon binding the metal ions. These conformations exhibit different degrees of FRET between the fluorophore (donor) and quencher (acceptor) at the termini of each DNA probe.


## EXPERIMENTAL SECTION

**Chemicals.** Acetic acid, 4-(2-hydroxyethyl)piperazine-1-ethanesulfonic acid hemisodium salt (HEPES), phytic acid, sodium cyanide (NaCN), tris(hydroxymethyl)aminomethane (Tris), and all of the metal salts used in this study were purchased from Aldrich (Milwaukee, WI). The TBA probe (Fam–5'-GGTGGTGTGGTTGG-3'-DABCYL) and the random DNA (5'-ATGTACCGATCACTA-3') were purchased from Integrated DNA Technology, Inc. (Coralville, IA). Montana Soil (SRM 2710) was obtained from the National Institute of Standards and Technology (NIST, Maryland). Milli-Q ultrapure water was used in each experiment. The toxic sodium cyanide was used with caution because it is a potent inhibitor of respiration.

**Analysis of Samples.** For lead sensing, aliquots (500 μL) of 10 mM Tris–acetate (pH 7.4) solutions containing the TBA probe (10 nM), Pb<sup>2+</sup> (0–1.0 μM), NaCN (100 μM), and the random blocking DNA (100 nM) were equilibrated at room temperature for 15 min prior to measurement of the fluorescence. In this




**Figure 1.** Fluorescence spectra of solutions of (a) TBA probe (10 nM) and (b and c) TBA probe (10 nM) in the presence of (b) Pb<sup>2+</sup> (100 nM) and (c) Hg<sup>2+</sup> (500 nM). Buffer, 10 mM Tris–acetate (pH 7.4); excitation wavelength, 475 nm. The fluorescence intensities ( $I_F$ ) are plotted in arbitrary units (a. u.).



**Figure 2.** Ellipticity plotted with respect to the (A) Pb<sup>2+</sup> ion concentration (0, 0.2, 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, and 5.0 μM) and (B) Hg<sup>2+</sup> ion concentration (0, 2.5, 5.0, 7.5, 10, 15, 20, and 25 μM). Each sample was prepared in 10 mM Tris–acetate (pH 7.4) containing 5.0 μM TBA probe.

paper, the final concentrations of the species are provided. For mercury sensing, aliquots (500 μL) of 10 mM Tris–acetate (pH 7.4) solutions containing the TBA probe (10 nM), Hg<sup>2+</sup> (0–1.0 μM), and phytic acid (100 μM) were equilibrated at room temperature for 15 min prior to measurement of the fluorescence using a fluorescence spectrophotometers (Cary Eclipse; Varian, California). The fluorescence lifetime of the TBA probe in the absence and presence of the two metal ions were measured using a Edinburgh FL 900 photon-counting system (Edinburgh, U.K.), and then the data were treated by fitting to a biexponential fluorescence decay. Acidic digestion of soil samples (1 g) was performed according to EPA method 305B.<sup>12</sup> Aliquots (50 μL) of the diluted soil samples (0.0001×) were spiked with standard solutions of Pb<sup>2+</sup> over the concentration

- (10) (a) Kotch, F. W.; Fettinger, J. C.; Davis, J. T. *Org. Lett.* **2000**, *2*, 3277–3280. (b) Smirnov, I.; Shafer, R. H. *J. Mol. Biol.* **2000**, *296*, 1–5. (c) Smirnov, I. V.; Kotch, F. W.; Pickering, I. J.; Davis, J. T.; Shafer, R. H. *Biochemistry* **2002**, *41*, 12133–12139.
- (11) (a) Katz, S. *J. Am. Chem. Soc.* **1952**, *74*, 2238–2245. (b) Yamane, T.; Davidson, N. *J. Am. Chem. Soc.* **1961**, *83*, 2599–2607. (c) Miyake, Y.; Togashi, H.; Tashiro, M.; Yamaguchi, H.; Oda, S.; Kudo, M.; Tanaka, Y.; Kondo, Y.; Sawa, R.; Fujimoto, T.; Machinami, T.; Ono, A. *J. Am. Chem. Soc.* **2006**, *128*, 2172–2173. (d) Tanaka, Y.; Oda, S.; Yamaguchi, H.; Kondo, Y.; Kojima, C.; Ono, A. *J. Am. Chem. Soc.* **2007**, *129*, 244–245.
- (12) *Test Methods for Evaluating Solid Waste, Physical/Chemical Methods*, 3rd ed.; USEPA SW-846, U.S. Government Printing Office: Washington, DC, 1996.

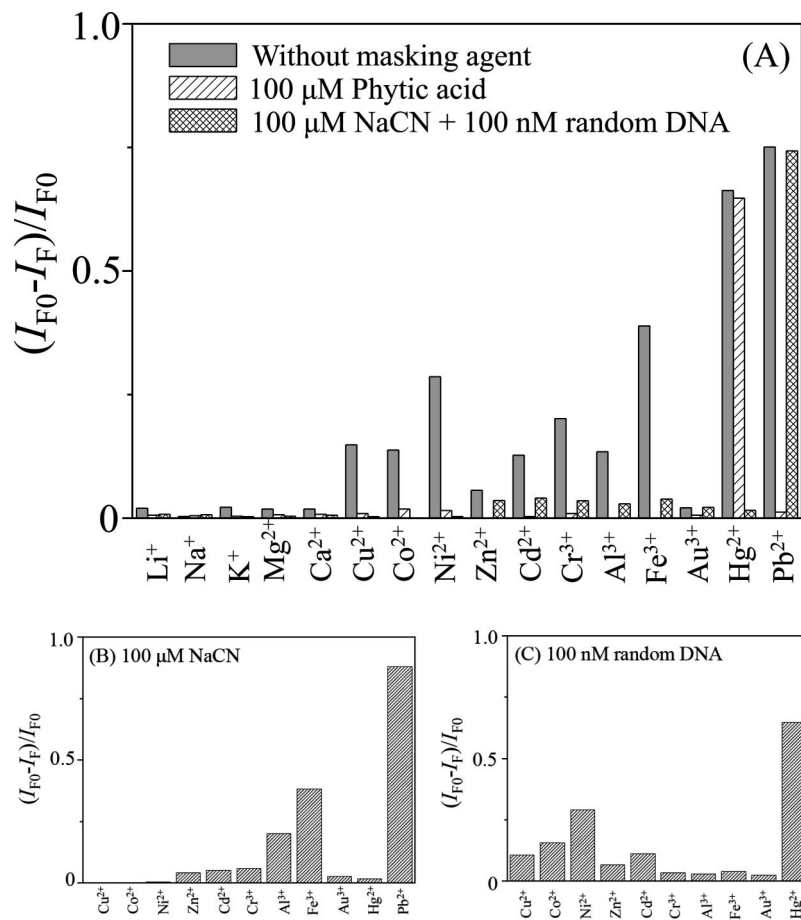

**Figure 3.** Quenching efficiency  $(I_{F0} - I_F)/I_{F0}$  of the fluorescence intensity (518 nm) of the probe in the presence of metal ions in the absence and presence of masking agents. (A) Concentrations: Hg<sup>2+</sup>, 1.0 μM; Pb<sup>2+</sup>, 100 nM; Li<sup>+</sup> and Na<sup>+</sup>, 100 μM; K<sup>+</sup>, Mg<sup>2+</sup>, and Ca<sup>2+</sup>, 10 μM; other ions, 1.0 μM. (B and C) metal ions (1.0 μM) in the presence of NaCN (100 μM) and random DNA (100 nM), respectively.


range of 10–500 nM. Prior to analysis, the mixtures were diluted to 500 μL with 10 mM Tris–acetate (pH 7.4) solution containing the TBA probe (10 nM), NaCN (100 μM), and the random blocking DNA (100 nM). A water sample collected from a pond on the campus of National Taiwan University was filtered through a 0.2 μm membrane. Aliquots of the pond water (490 μL) were spiked with standard Hg<sup>2+</sup> solutions (10 μL) at concentrations over the range of 10–500 nM. The spiked samples were then diluted to 1000 μL with 10 mM Tris–acetate (pH 7.4, 500 μL) containing 10 nM TBA probe and 100 μM phytic acid. The spiked samples were then analyzed separately using ICPMS and the present sensing technique.

## RESULTS AND DISCUSSION

**Sensing Strategy.** Scheme 1 displays the sensing strategy of the TBA probe toward the two target metal ions (Pb<sup>2+</sup> and Hg<sup>2+</sup>). The TBA has a random coil structure that changes into a G-quartet structure<sup>10</sup> and a hairpin-like structure structure<sup>11</sup> upon binding Pb<sup>2+</sup> and Hg<sup>2+</sup> ions, respectively. The TBA consists of nine deoxyguanosine (G) units, which interact specifically with Pb<sup>2+</sup> ions to form a G-quadruplex and six T units, which bind to Hg<sup>2+</sup> ions through T–Hg<sup>2+</sup>–T interactions. As a result of the decreased distance between the donor and acceptor moieties—and, hence, FRET between the FAM and DABCYL units—the fluorescence of FAM in the presence of Pb<sup>2+</sup> or Hg<sup>2+</sup> is weak. We performed proof-of-concept experiments for the detection of Pb<sup>2+</sup> and Hg<sup>2+</sup> ions using the TBA

probe (10 nM). Curve a in Figure 1 indicates that the fluorescence of the solution containing the TBA probe was strong in the absence of the two metal ions, consistent with the fact that the TBA probe exists in a random coiled structure. After separately adding Pb<sup>2+</sup> (100 nM) and Hg<sup>2+</sup> (500 nM) to the probe solution, the fluorescence at 518 nm (excitation at 475 nm) decreased to different degrees, as curves b and c indicate, respectively. The greater decrease in fluorescence (i.e., greater FRET efficiency) in the presence of Pb<sup>2+</sup> than that in the presence of Hg<sup>2+</sup> reveals that the donor and acceptor are positioned relatively closer in the G-quartet structure. CD spectra (Figure 2) confirmed the formation of G-quadruplex and hairpin-like structure structures from the TBA probe in the presence of Pb<sup>2+</sup> and Hg<sup>2+</sup>, respectively.<sup>10,11</sup>

In order to further investigate the impacts of Pb<sup>2+</sup> and Hg<sup>2+</sup> on the fluorescence changes, we compared the lifetimes of the probe in the absence and presence of the metal ions. The lifetimes of the TBA, Hg<sup>2+</sup>/TBA, and Pb<sup>2+</sup>/TBA were 2.1, 1.1, and 0.8 ns, respectively. We also compared the fluorescence quenching efficiencies of the probe separately in the presence of Pb<sup>2+</sup> and Hg<sup>2+</sup> at the same concentration. The quenching efficiencies of Pb<sup>2+</sup> and Hg<sup>2+</sup> (both at 500 nM) were 81% and 66%, respectively. The results reveal that the distance of the two fluorophores in the TBA in the presence of Pb<sup>2+</sup> was closer than that of Hg<sup>2+</sup>.



**Figure 4.** Quenching efficiency plotted with respect to the (A)  $\text{Hg}^{2+}$ , (B)  $\text{Pb}^{2+}$ , and (C)  $\text{K}^{+}$  ion concentrations. The solution contained  $\text{K}^{+}$  and interference metal ions ( $\text{Pb}^{2+}$ ,  $100.0 \text{ nM}$ ;  $\text{Hg}^{2+}$ ,  $500.0 \text{ nM}$ ) in the presence of (a) phytic acid ( $100 \mu\text{M}$ ), (b) NaCN ( $100 \mu\text{M}$ ) and random DNA ( $100 \text{ nM}$ ), and (c) phytic acid ( $100 \mu\text{M}$ ), NaCN ( $100 \mu\text{M}$ ), and random DNA ( $100 \text{ nM}$ ).

**Buffer Composition, Masking Agents, and Selectivity.** We carefully tested the detection of  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  using our probe in four different buffer systems ( $10 \text{ mM}$ ,  $\text{pH } 7.4$ ), including Tris–acetate, HEPES, sodium acetate, and sodium phosphate. The values of  $[(I_{F0} - I_F)/I_{F0}]$  for the solutions buffered with sodium phosphate, HEPES, Tris–acetate, and sodium acetate at  $1.0 \mu\text{M}$   $\text{Pb}^{2+}$  were  $0.25$ ,  $0.78$ ,  $0.80$ , and  $0.81$ , respectively. Herein,  $I_F$  and  $I_{F0}$  represent fluorescence intensity in the presence and absence of the metal ion, respectively. The values of  $[(I_{F0} - I_F)/I_{F0}]$  for the solutions buffered with sodium phosphate, HEPES, Tris–acetate, and sodium acetate at  $1.0 \mu\text{M}$   $\text{Hg}^{2+}$  were  $0.68$ ,  $0.66$ ,  $0.69$ , and  $0.68$ , respectively (data not shown). The sensitivity decreased upon increasing the stability of metal–anion complexes; for example, we obtained lower sensitivity for  $\text{Pb}^{2+}$  in phosphate buffer than that in Tris–acetate buffer (formation constants:  $\text{p}K_f = 43.5$  for  $\text{Pb}_3\text{L}_2$  (L, phosphate) and  $\text{p}K_f = 4.1$  for  $\text{PbL}_2$  (L, acetate;  $\text{p}K_f = 10.1$  for  $\text{HgL}_2$ ).

To investigate the selectivity of the TBA probe toward these two metal ions, we added  $100 \text{ nM}$   $\text{Pb}^{2+}$  and  $\text{Hg}^{2+}$ ,  $100 \mu\text{M}$   $\text{Li}^{+}$  and  $\text{Na}^{+}$ ,  $10 \mu\text{M}$   $\text{K}^{+}$ ,  $\text{Mg}^{2+}$ , and  $\text{Ca}^{2+}$ , and  $100 \text{ nM}$   $\text{Cu}^{2+}$ ,  $\text{Co}^{2+}$ ,  $\text{Ni}^{2+}$ ,  $\text{Zn}^{2+}$ ,  $\text{Cd}^{2+}$ ,  $\text{Cr}^{3+}$ ,  $\text{Al}^{3+}$ ,  $\text{Fe}^{3+}$ , and  $\text{Au}^{3+}$  separately into the probe solutions. Only  $\text{Pb}^{2+}$  and  $\text{Hg}^{2+}$  caused decreases in the fluorescence of FAM (data not shown), revealing that the probe is selective for  $\text{Pb}^{2+}$  and  $\text{Hg}^{2+}$  ions. High concentrations ( $>1.0 \mu\text{M}$ ) of  $\text{Cu}^{2+}$ ,  $\text{Co}^{2+}$ ,  $\text{Ni}^{2+}$ ,  $\text{Cd}^{2+}$ ,  $\text{Cr}^{3+}$ ,  $\text{Al}^{3+}$ , and  $\text{Fe}^{3+}$  ions, however, decreased the fluorescence of FAM, leading to false-

positive signals (Figure 3A). To overcome this problem, we tested the effects of several masking reagents, including phytic acid,  $\text{CN}^{-}$ , and a random DNA strand. It is well-known that phosphate ions form stable complexes with several metal ions, including  $\text{Fe}^{2+}$ ,  $\text{Co}^{2+}$ ,  $\text{Ni}^{2+}$ ,  $\text{Cu}^{2+}$ ,  $\text{Zn}^{2+}$ , and  $\text{Pb}^{2+}$ . Thus, we tested the masking capability of phytic acid for the interfering metal ions in our sensing system. Gratifyingly, only  $\text{Hg}^{2+}$  caused a decrease in the fluorescence of FAM in the presence of  $100 \mu\text{M}$  phytic acid (Figure 3A); i.e., this sensing system is specific to  $\text{Hg}^{2+}$ . For example, in  $10 \text{ mM}$  Tris–acetate solution ( $\text{pH } 7.4$ ) containing  $100 \mu\text{M}$  phytic acid, the TBA probe provided high selectivity (50-fold or more) toward  $\text{Hg}^{2+}$  ions over the other metal ions. To improve the selectivity of the TBA probe toward  $\text{Pb}^{2+}$ , we added  $\text{CN}^{-}$  as a masking agent because it forms a much more stable complex with  $\text{Hg}^{2+}$  ions ( $\log \beta_2 = 32.8$ ) than with  $\text{Pb}^{2+}$  ions.<sup>13</sup> As indicated in Figure 3B, the presence of  $\text{CN}^{-}$  masked the TBA probe toward other ions but not toward  $\text{Pb}^{2+}$ ,  $\text{Al}^{3+}$ , or  $\text{Fe}^{3+}$ . To mask the two trivalent metal ions, we added a random DNA sample ( $100 \text{ nM}$ ) having the sequence 5'-ATGTACCGATCACTA-3'. Figure 3C reveals that the random DNA did not mask  $\text{Pb}^{2+}$ , but it did mask the  $\text{Al}^{3+}$  and  $\text{Fe}^{3+}$  ions by at least 78% and 90%, respectively. The random DNA interacted with the two interfering metal ions through electrostatic attractions. The interactions between  $\text{Pb}^{2+}$  and the random DNA are much weaker than those with TBA (G-quadruplex). In  $10 \text{ mM}$  Tris–acetate solution ( $\text{pH } 7.4$ ) containing  $100 \mu\text{M}$  NaCN and  $100 \text{ nM}$  of the random DNA, the TBA probe provided high selectivity (400-fold or more) toward  $\text{Pb}^{2+}$  ions over all of the other tested interference ions (Figure 3A).

Different possible interferences including anions and thiol compounds were also tested. We found that  $\text{Cl}^{-}$ ,  $\text{Br}^{-}$ ,  $\text{F}^{-}$ ,  $\text{NO}_3^{-}$ ,  $\text{SO}_4^{2-}$ , and  $\text{CO}_3^{2-}$  (all sodium salts), respectively, did not interfere the detection of  $\text{Pb}^{2+}$  and  $\text{Hg}^{2+}$ . However, when the concentration of NaCl increased from  $10$  to  $100 \text{ mM}$ , the value of  $[(I_{F0} - I_F)/I_{F0}]$  for the solution increased from  $0.02$  to  $0.25$ , mainly due to the formation of G-quartet under the high-salt conditions. We also found that thiol compounds, such as sodium sulfide, potassium peroxydisulfate, ethanethiol, and thiourea at high concentrations caused interferences in sensing  $\text{Pb}^{2+}$  and  $\text{Hg}^{2+}$ . The tolerance concentration of these four thiol compounds for detecting  $\text{Pb}^{2+}$  and  $\text{Hg}^{2+}$  were all  $100$  and  $10 \mu\text{M}$ , respectively. The tolerance concentration is defined by 50% decreases in the intensity of  $(I_{F0} - I_F)/I_{F0}$  when the interference is present.

**Sensitivity and Application.** Under the optimal conditions, we investigated the sensitivity of the TBA probe toward  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  individually. The fluorescence of FAM decreased upon increasing the concentration of  $\text{Hg}^{2+}$  (Figure 4A) or  $\text{Pb}^{2+}$  (Figure 4B). We obtained linear responses of the expression  $(I_{F0} - I_F)/I_{F0}$  against the concentrations of  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  over the ranges of  $10$ – $200 \text{ nM}$  ( $R^2 = 0.98$ ) and  $0.5$ – $30 \text{ nM}$  ( $R^2 = 0.98$ ), respectively. The TBA probe provided limits of detection (LODs) for  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  ions (signal-to-noise ratio = 3) of  $5.0 \text{ nM}$  and  $300 \text{ pM}$ , respectively. Thus, this approach provides a sensitivity toward  $\text{Pb}^{2+}$  ions that is more than 1 order of magnitude lower than that reported when using a DNAzyme.<sup>6</sup>

(13) Morel, F. M. M. *Principles of Aquatic Chemistry*; Wiley: New York, 1983.

In addition, this TBA probe provides a sensitivity for  $\text{Hg}^{2+}$  ions that is comparable to that of a system we reported previously.<sup>7b,9c</sup> Our results suggested that this TBA probe would be sensitive for monitoring the levels of  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  ions in foodstuffs and environmental samples. For example, the U.S. Food and Drug Administration suggests an action level for lead of  $2.5\ \mu\text{M}$  (500 ppb) in products intended for children; the U.S. Environmental Protection Agency permits the maximum level of mercury in drinking water to be 10 nM (2.0 ppb). In addition, we also demonstrated that our sensor provides selective detection of  $\text{K}^+$  in the presence of masking agents, phytic acid, NaCN, and random DNA (Figure 4C). The linear range of fluorescence response of our sensor for  $\text{K}^+$  was about 0.1–10 mM.

Thus, we used our TBA probe to determine the concentrations of  $\text{Pb}^{2+}$  and  $\text{Hg}^{2+}$  in soil and pond water samples, respectively. The concentrations of lead determined ( $n = 5$ ) using our new approach and ICPMS were  $5.28 (\pm 0.07)$  and  $5.05 (\pm 0.10)$  mg/g, respectively. The  $F$ -test value for the correlation between the two methods was 2.04 (the  $F$ -test value is 6.39 at a 95% confidence level), suggesting that the two methods did not differ significantly. We obtained a linear correlation ( $R^2 = 0.97$ ) between the responses and the concentration of  $\text{Hg}^{2+}$  ions spiked into the pond water over the range of 10–200 nM. The TBA probe provided recoveries of 95–104% for these measurements. Neither our probe nor the ICPMS system detected the presence of  $\text{Hg}^{2+}$  ions in the pond water sample. These results

reveal the practicality of using our TBA probe for the determination of  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  ions in environmental samples.

## CONCLUSION

In conclusion, we have devised a new assay for the sensitive and selective detection of  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  ions using an aptamer (TBA) that interacts specifically with thrombin. Changes in the DNA strand's conformation allowed us to readily detect  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  using this TBA probe in the presence of phytic acid and a random DNA/NaCN mixture, respectively. The practicality of this method has been validated by the analyses of soil and water samples. To the best of our knowledge, this is the first example of a single DNA-based sensor that allows the detection of both  $\text{Hg}^{2+}$  and  $\text{Pb}^{2+}$  ions. The simple, rapid, and cost-effective sensing systems hold great practical for detection of heavy metal ions in real samples.

## ACKNOWLEDGMENT

This study was supported by the National Science Council of Taiwan under contracts NSC-95-2113-M-002-026-MY3, NSC 97-2627-M-002-010, and NSC 97-2627-M-002-011.

Received for review October 19, 2008. Accepted January 26, 2009.

AC8022185